



TL-941



中国认可
国际互认
检测
TESTING
CNAS L5868



Test Report



Report No.: MTI201207005P002

Date of Issue: 2020.12.18

Client: Shenzhen HJR Electronics Technology Co.,LTD.

Product: Particle filtering half mask

Test Type: Commissioned Inspection



Shenzhen Microtest Co., Ltd.

<http://www.mtitest.com>



Tel: (86-755)88850135

Fax: (86-755) 88850136

Web:www.mtitest.com

E-mail: mti@51mti.com

Address: 101, No. 7, Zone 2, Xinxing Industrial Park, Fuhai Avenue, Xinhe Community, Fuhai Street, Bao' an District, Shenzhen, Guangdong, China.



Instructions


1. The report shall not be partially reproduced without the written consent of the Laboratory ;
2. The test results of this report are only responsible for the samples submitted ;
3. This report is invalid without the seal and signature of the laboratory ;
4. This report is invalid if transferred, altered or tampered with in any form without authorization ;
5. Any objection to this report shall be submitted to the laboratory within 15 days from the date of receipt of the report.



TEST REPORT

Report No.: MTI201207005P002

Page 1 of 8

Basic Information			
Client	Shenzhen HJR Electronics Technology Co.,LTD.		
Client Address	5 / F Building A3 Xinjianxing Science and Technology Industrial Park, No. 3333, Guangqiao Avenue, Gongming Street, Guangming New District, Shenzhen City, Guangdong Province, China		
Manufacturer	Shenzhen HJR Electronics Technology Co.,LTD.		
Manufacturer Address	5 / F Building A3 Xinjianxing Science and Technology Industrial Park, No. 3333, Guangqiao Avenue, Gongming Street, Guangming New District, Shenzhen City, Guangdong Province, China		
Sample Information			
Product	Particle filtering half mask	Sample No.	MTI201207005-1-S000 2
Brand/Trademark		Model	HJR-CN99-12
Sample Number	80 Pcs	Sample Description	Blue ear wearing type, folding type mask
Testing Information			
Sample Receive Date	2020.12.14	Sample Source	Customer provided
Test Specification	EN 149:2001+A1:2009		
Classification	FFP2		
Date of Tests	2020.12.14~2020.12.18		
Test Address	Medical protection laboratory		
Test Result	The sample has been tested and the test items meet the requirements of EN 149:2001+A1:2009.		
Remarks	"/" in the report means this item is blank,"N/A" in the report means this item is not application.		
Compiled:	<i>Hong Pu</i>	Reviewed:	<i>Daniel Shi</i>
		Approved:	<i>Tom Xue</i>

No.	Test Items	Spec Chapter	Requirements	Test Data	Assesment
1	Visual inspection	7.3	The visual inspection shall also include the marking and the information supplied by the manufacturer.	Meet the requirements.	Pass
2	Material	7.5	Meet the requirements of 7.5	Meet the requirements.	Pass
3	Practical performance	7.7	The particle filtering half mask shall undergo practical performance tests under realistic conditions.	Meet the requirements.	Pass
4	Finish of parts	7.8	Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs.	Meet the requirements.	Pass
5	Total inward leakage	7.9.1	For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than: 25 % for FFP1, 11 % for FFP2, 5 % for FFP3 . and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than: 22 % for FFP1, 8 % for FFP2, 2 % for FFP3.	Test results are shown in Annex A Table 7.9.1-A&B.	Pass
6	Penetration of filter material	7.9.2	Sodium chloride test 95l/min: FFP1 ≤ 20%, FFP2 ≤ 6%, FFP3 ≤ 1%. Paraffin oil test 95l/min: FFP1 ≤ 20%, FFP2 ≤ 6%,	Test results are shown in Annex A Table 7.9.2.	Pass

			FFP3≤1%.		
7	Compatibility with skin	7.10	Materials that may come into contact with the wearer's skin shall not be known to be likely to cause irritation or any other adverse effect to health.	Meet the requirements.	Pass
8	Flammability	7.11	When tested, the particle filtering half mask shall not burn or not to continue to burn for more than 5 s after removal from the flame.	A.R.: 29#:not burn 30#: not burn T.C.: 31#: not burn 32#: not burn	Pass
9	Carbon dioxide content of the inhalation air	7.12	The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume).	A.R.: 33#:0.62% 34#:0.64% 35#:0.64% Mean:0.63%	Pass
10	Head harness	7.13	Meet the requirements of 7.13	Meet the requirements.	Pass
11	Field of vision	7.14	The field of vision is acceptable if determined so in practical performance tests.	Meet the requirements.	Pass
12	Exhalation valve(s)	7.15	Meet the requirements of 7.15	Only applicable to Exhalation valve(s) Particle filtering half mask.	N/A
13	Breathing resistance	7.16	Inhalation 30 l/min:FFP1≤0.6mbar,FFP2≤0.7 mbar,FFP3≤1.0mbar. Inhalation 95 l/min:FFP1≤2.1mbar,FFP2≤2.4 mbar,FFP3≤3.0mbar. Exhalation 160 l/min:FFP1≤3.0mbar,FFP2≤3.0 mbar,FFP3≤3.0mbar.	Test results are shown in Annex A Table 7.16.	Pass
14	Demountable parts	7.18	All demountable parts (if fitted) shall be readily connected and	/	N/A



TEST REPORT



Report No.: MTI201207005P002

Page 4 of 8

			secured, where possible by hand.		
Note: A.R.:As received		S.W.: Simulated wearing treatment		M.S.:Mechanical strength	
T.C.:Temperature conditioning		F.C.:Flow conditioning			

Item Name	File No	Uncertainty	
Penetration of filter material	MTI-SOP-PH-U005	$U_{rel} = 2.1\%, k=2$	
Carbon dioxide content of the inhalation air	MTI-SOP-PH-U007	$U_{rel} = 1.8\%, k=2$	
Total inward leakage	MTI-SOP-PH-U008	$U_{rel} = 1.8\%, k=2$	
Breathing resistance	MTI-SOP-PH-U006	30L/min	$U_{rel} = 2.5\%, k=2$
		95L/min	$U_{rel} = 2.4\%, k=2$
		160L/min	$U_{rel} = 2.3\%, k=2$



Annex A: Summarization of Test Data

Tel: (86-755)88850135

Fax: (86-755) 88850136

Web: www.mttest.com

E-mail: mti@51mti.com

Address: 101, No. 7, Zone 2, Xinxing Industrial Park, Fuhai Avenue, Xinhe Community, Fuhai Street, Bao 'an District, Shenzhen, Guangdong, China.

TEST REPORT

Report No.: MTI201207005P002

Page 5 of 8

Table 7.9.1-A Total inward leakage test data

Test specification: EN 149:2001+A1:2009 Clause 8.5

Subject	No.	Condition	Walk(%)	Head Side/side(%)	Head Up/down(%)	Talk(%)	Walk(%)	Mean(%)
Elaine	1#	A.R.	3.59	7.03	6.61	4.46	4.32	5.20
Lani	2#	A.R.	2.78	5.37	5.48	3.94	4.15	4.34
Baron	3#	A.R.	2.79	4.53	4.03	7.40	3.34	4.42
Hong	4#	A.R.	2.60	3.34	2.51	3.81	3.91	3.23
Shane	5#	A.R.	2.40	2.43	3.40	2.48	2.47	2.64
Noak	6#	T.C.	2.62	3.24	2.86	1.96	3.17	2.77
Harper	7#	T.C.	2.94	1.90	5.44	2.90	4.12	3.46
Lucy	8#	T.C.	5.12	5.75	4.86	6.94	3.76	5.29
Carl	9#	T.C.	2.19	2.92	2.73	5.61	6.41	3.97
James	10#	T.C.	1.07	1.47	1.24	1.13	1.19	1.22

Table 7.9.1-B Facial dimension

Subject	Face Length (mm)	Face Width (mm)	Face Depth (mm)	Mouth Width (mm)
Elaine	102	142	103	59
Lani	135	150	130	51
Baron	110	140	105	56
Hong	106	138	115	57
Shane	110	142	122	60
Noak	110	138	115	57
Harper	133	149	116	65
Lucy	99	142	108	55
Carl	130	150	125	54
James	119	148	100	58

Table 7.9.2 Penetration of filter material

Test specification: EN 149:2001+A1:2009 Clause 8.11

Aerosol	Condition	Sample No.	Average penetration after 3min (%)	Maximum penetration during exposure (%)
Sodium chloride test Aerosol concentration: 10 mg/m ³	As received	11#	0.18	/
		12#	0.10	/
		13#	0.13	/
	Simulated wearing treatment	14#	0.02	/
		15#	0.03	/
		16#	0.03	/
	Mechanical strength+ Temperature conditioned	17#	/	0.14
		18#	/	0.09
		19#	/	0.13
Paraffin oil Test Aerosol concentration: 23 mg/m ³	As received	20#	0.38	/
		21#	0.28	/
		22#	0.16	/
	Simulated wearing treatment	23#	0.56	/
		24#	0.41	/
		25#	0.56	/
	Mechanical strength+ Temperature conditioned	26#	/	0.64
		27#	/	0.51
		28#	/	0.56

TEST REPORT

Report No.: MTI201207005P002

Page 7 of 8


Table 7.16 Breathing resistance(mbar)

Test specification: EN 149:2001+A1:2009 Clause 8.9

	Flow rate		36#					37#					38#				
			A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
As received	Inhalation	30 l/min	0.42	0.41	0.42	0.42	0.43	0.42	0.41	0.42	0.42	0.43	0.42	0.43	0.43	0.44	0.44
		95 l/min	1.27	1.27	1.27	1.28	1.28	1.29	1.28	1.28	1.29	1.30	1.28	1.28	1.29	1.30	1.29
	Exhalation	160l/min	2.57	2.56	2.56	2.57	2.58	2.59	2.58	2.58	2.59	2.60	2.61	2.62	2.62	2.61	2.60
Simulated Wearing treatment	Flow rate		39#					40#					41#				
	Inhalation	30 l/min	0.45	0.46	0.45	0.45	0.44	0.44	0.43	0.44	0.45	0.45	0.44	0.45	0.44	0.44	0.43
		95 l/min	1.31	1.30	1.31	1.31	1.32	1.30	1.30	1.31	1.31	1.32	1.31	1.31	1.32	1.32	1.33
	Exhalation	160l/min	2.60	2.61	2.61	2.62	2.62	2.61	2.63	2.62	2.62	2.61	2.59	2.59	2.60	2.60	2.61
Temperature conditioned	Flow rate		42#					43#					44#				
	Inhalation	30 l/min	0.43	0.44	0.43	0.43	0.42	0.41	0.42	0.41	0.41	0.40	0.42	0.44	0.43	0.43	0.42
		95 l/min	1.26	1.27	1.26	1.26	1.25	1.24	1.25	1.25	1.24	1.23	1.25	1.24	1.24	1.25	1.26
	Exhalation	160l/min	2.58	2.60	2.59	2.59	2.58	2.57	2.56	2.57	2.57	2.58	2.57	2.57	2.58	2.58	2.59

A: facing directly ahead; B: facing vertically upwards; C: facing vertically downwards; D: lying on the left side; E: lying on the right side

Pictures

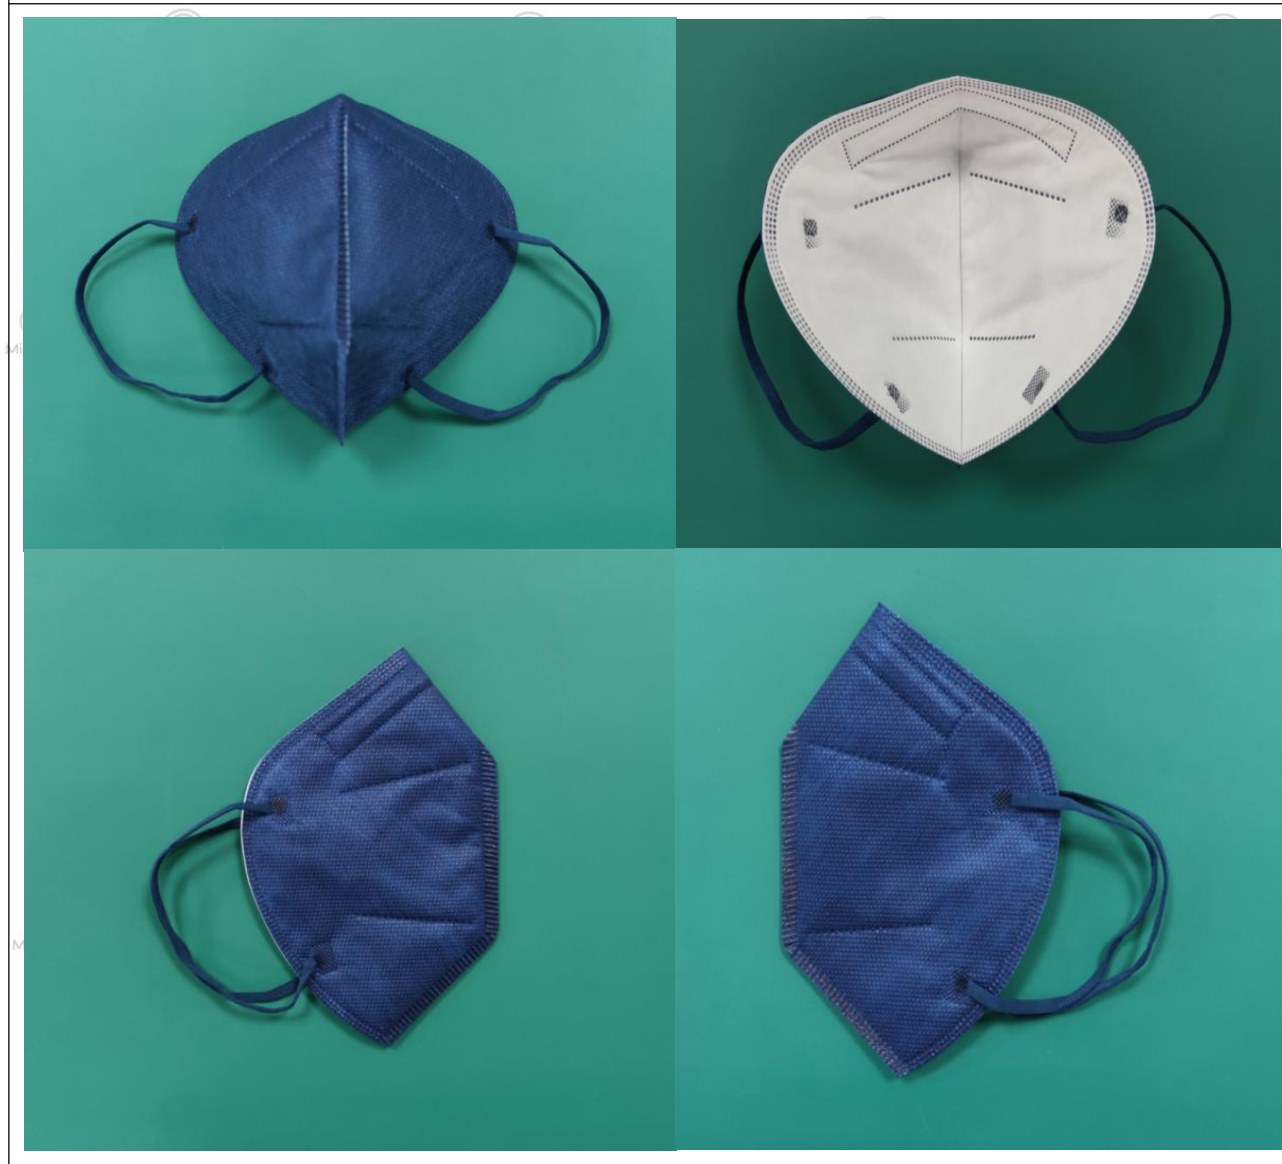

***** END *****